

6. NUCLEAR DISINTEGRATION AND RADIATION DETECTION

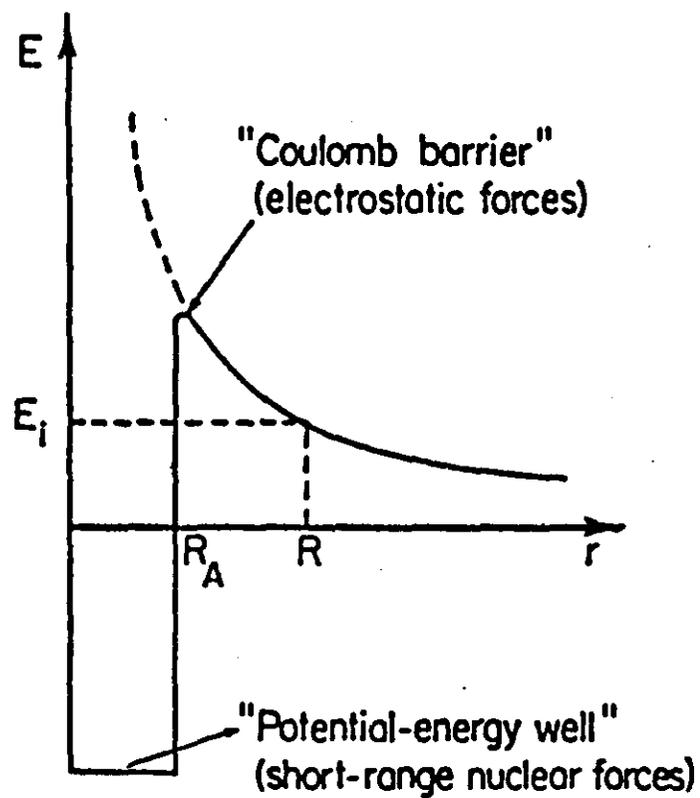


Fig. 6.1. Potential energy E as a function of the distance r from the nucleus. R_A is the nuclear radius.

$$P = \exp \left[-\frac{4\pi}{h} \sqrt{2m} \int_{R_A}^R \sqrt{U(r) - E_i} dr \right]$$

where h is Planck's constant, m is the reduced mass of the alpha particle

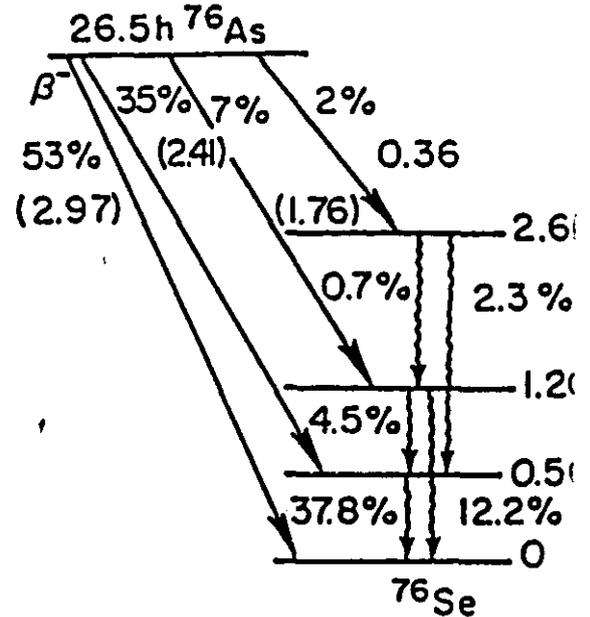
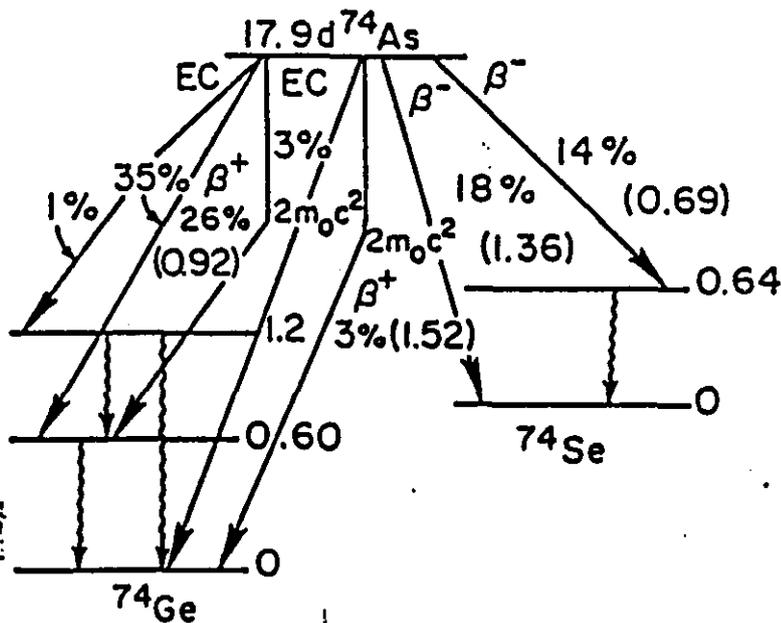
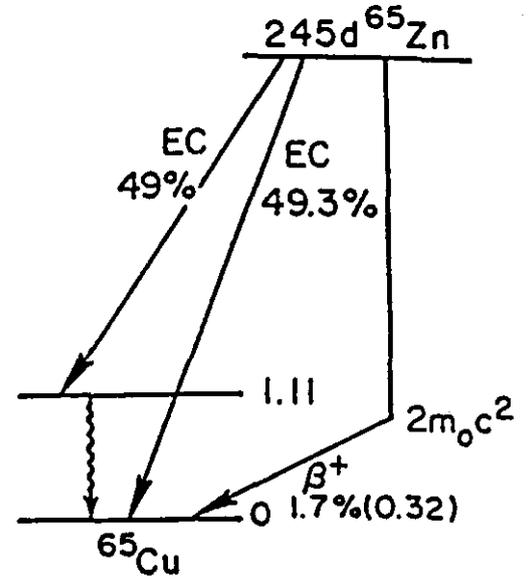
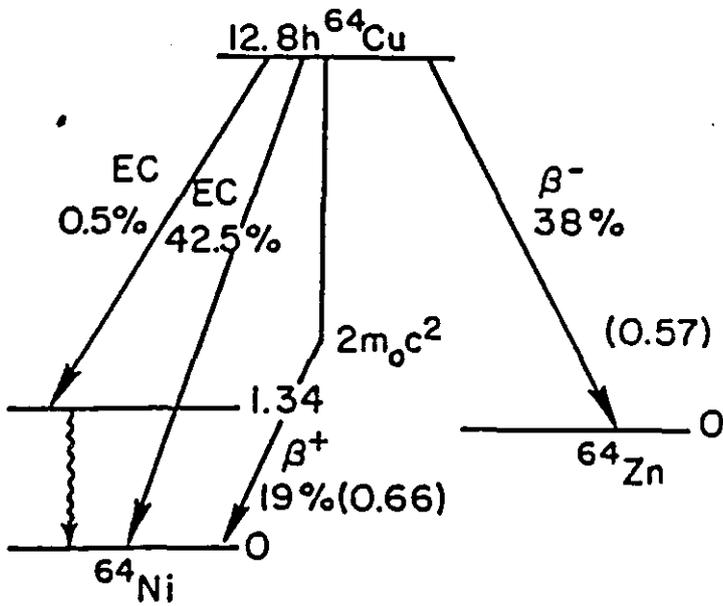


Figure 4.2 Decay schemes of some nuclides with complex modes of disintegration. Quantitative measurement of these radionuclides may be made by selecting the type and energy of a particular radiation and correcting the disintegration rate for the fraction of decays by that radiation.

6.1a

6.4a

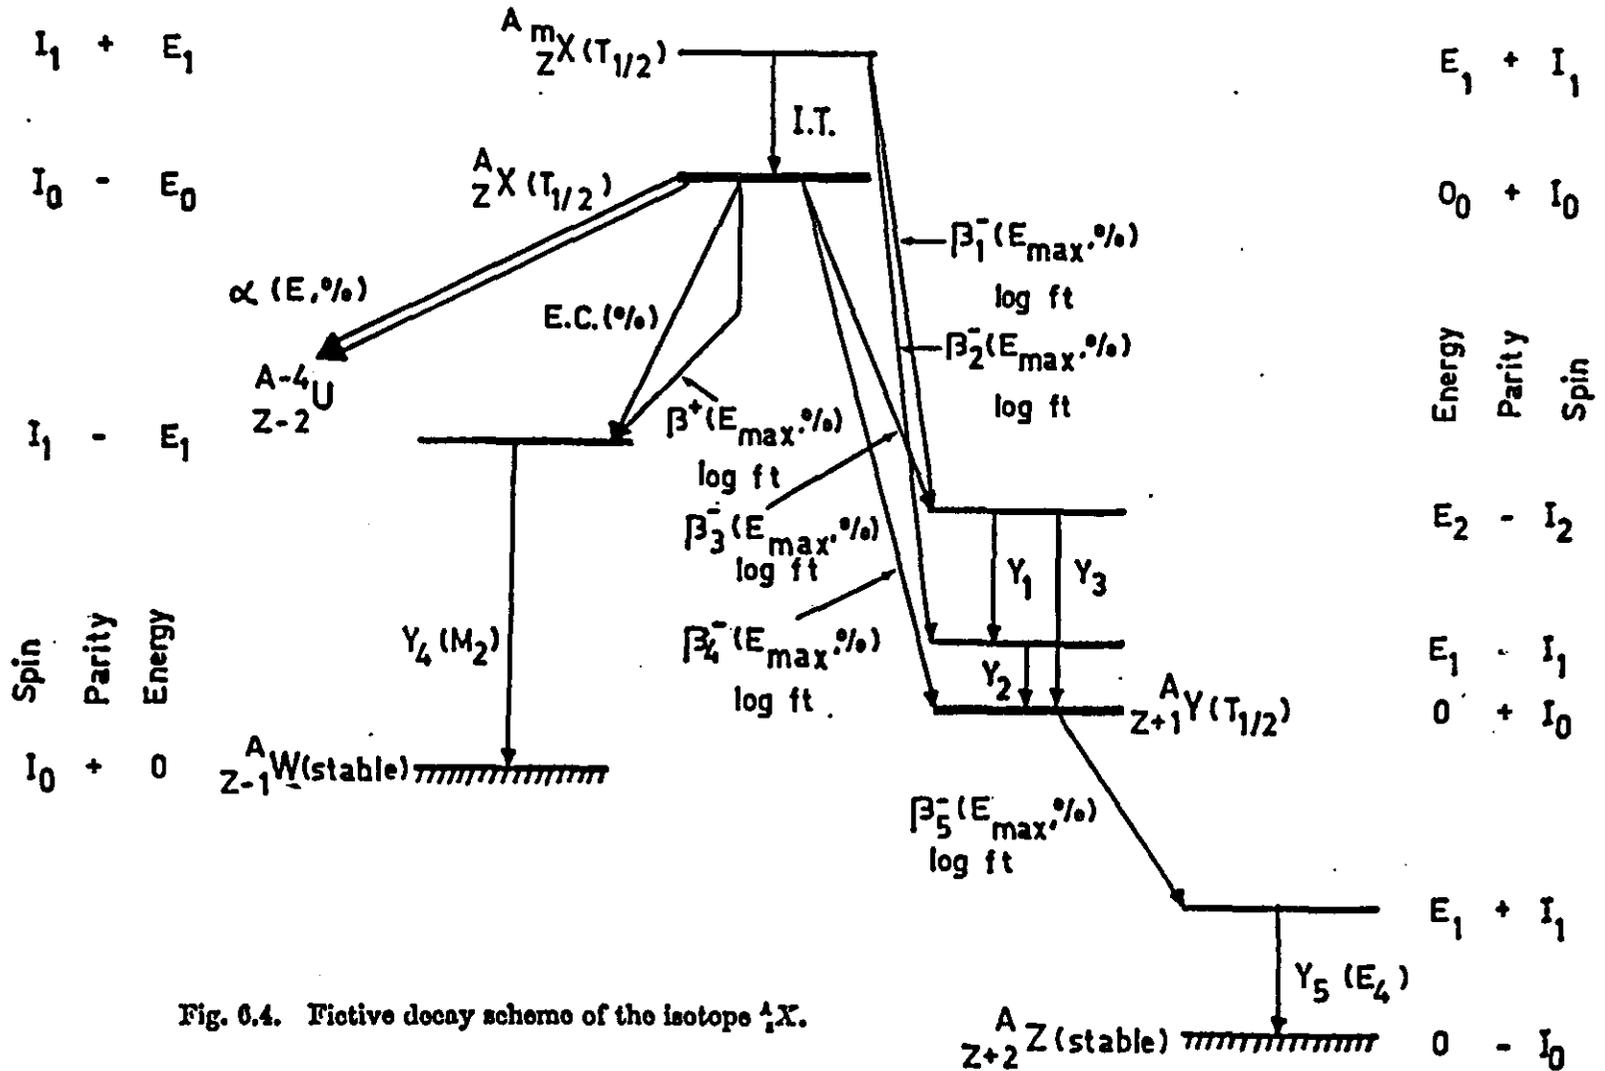


Fig. 6.4. Fictive decay scheme of the isotope ${}^A_Z X$.

6.18

6. NUCLEAR DISINTEGRATION AND RADIATION DETECTION

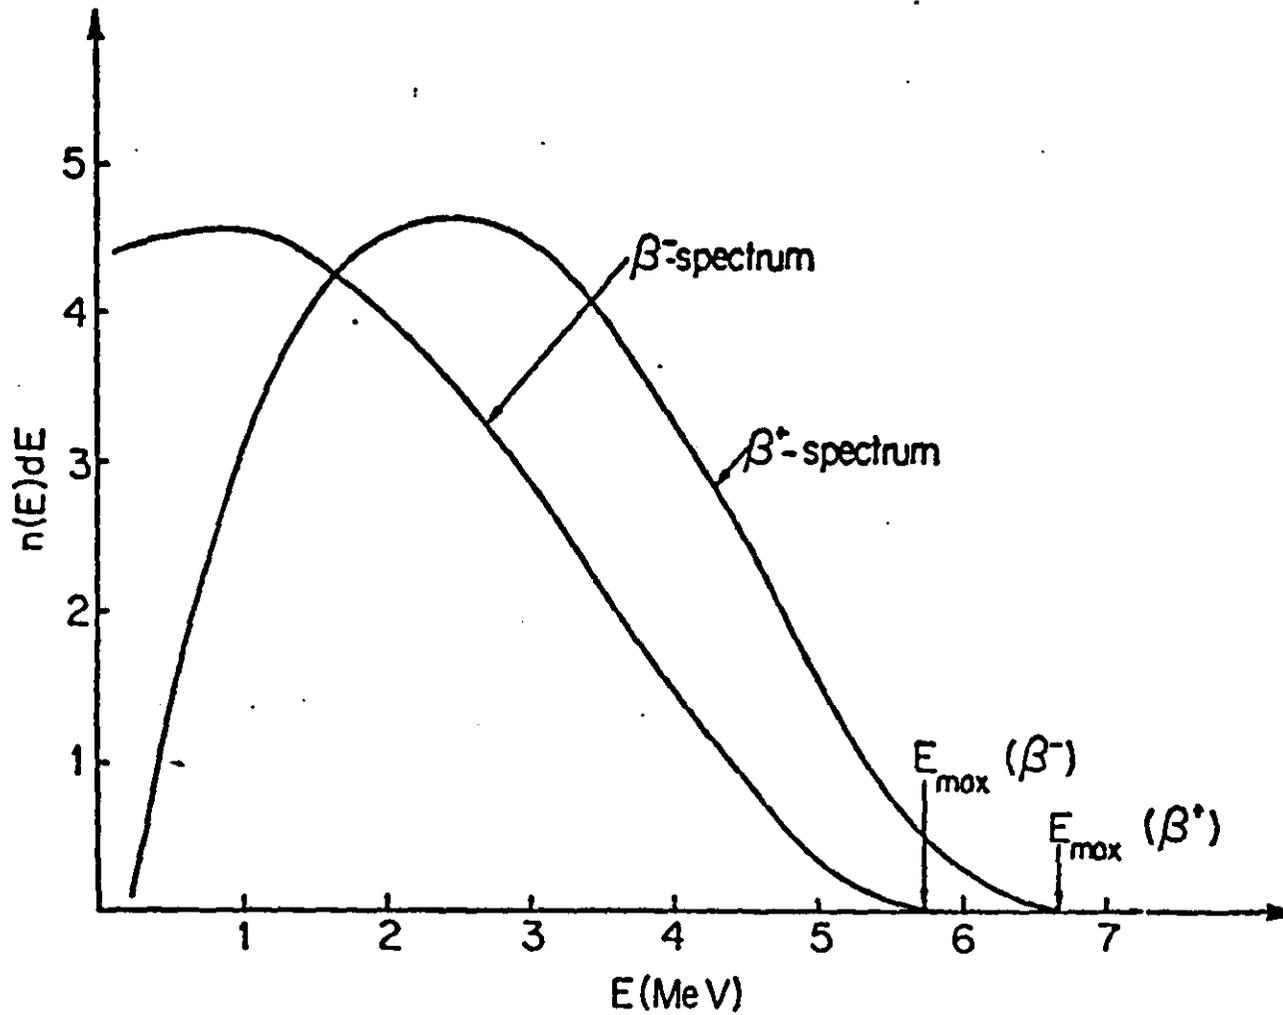


Fig. 6.2. Electron and positron spectrum of the isotope ^{64}Cu (8).

Radiochemistry and Radioactivity Measurement


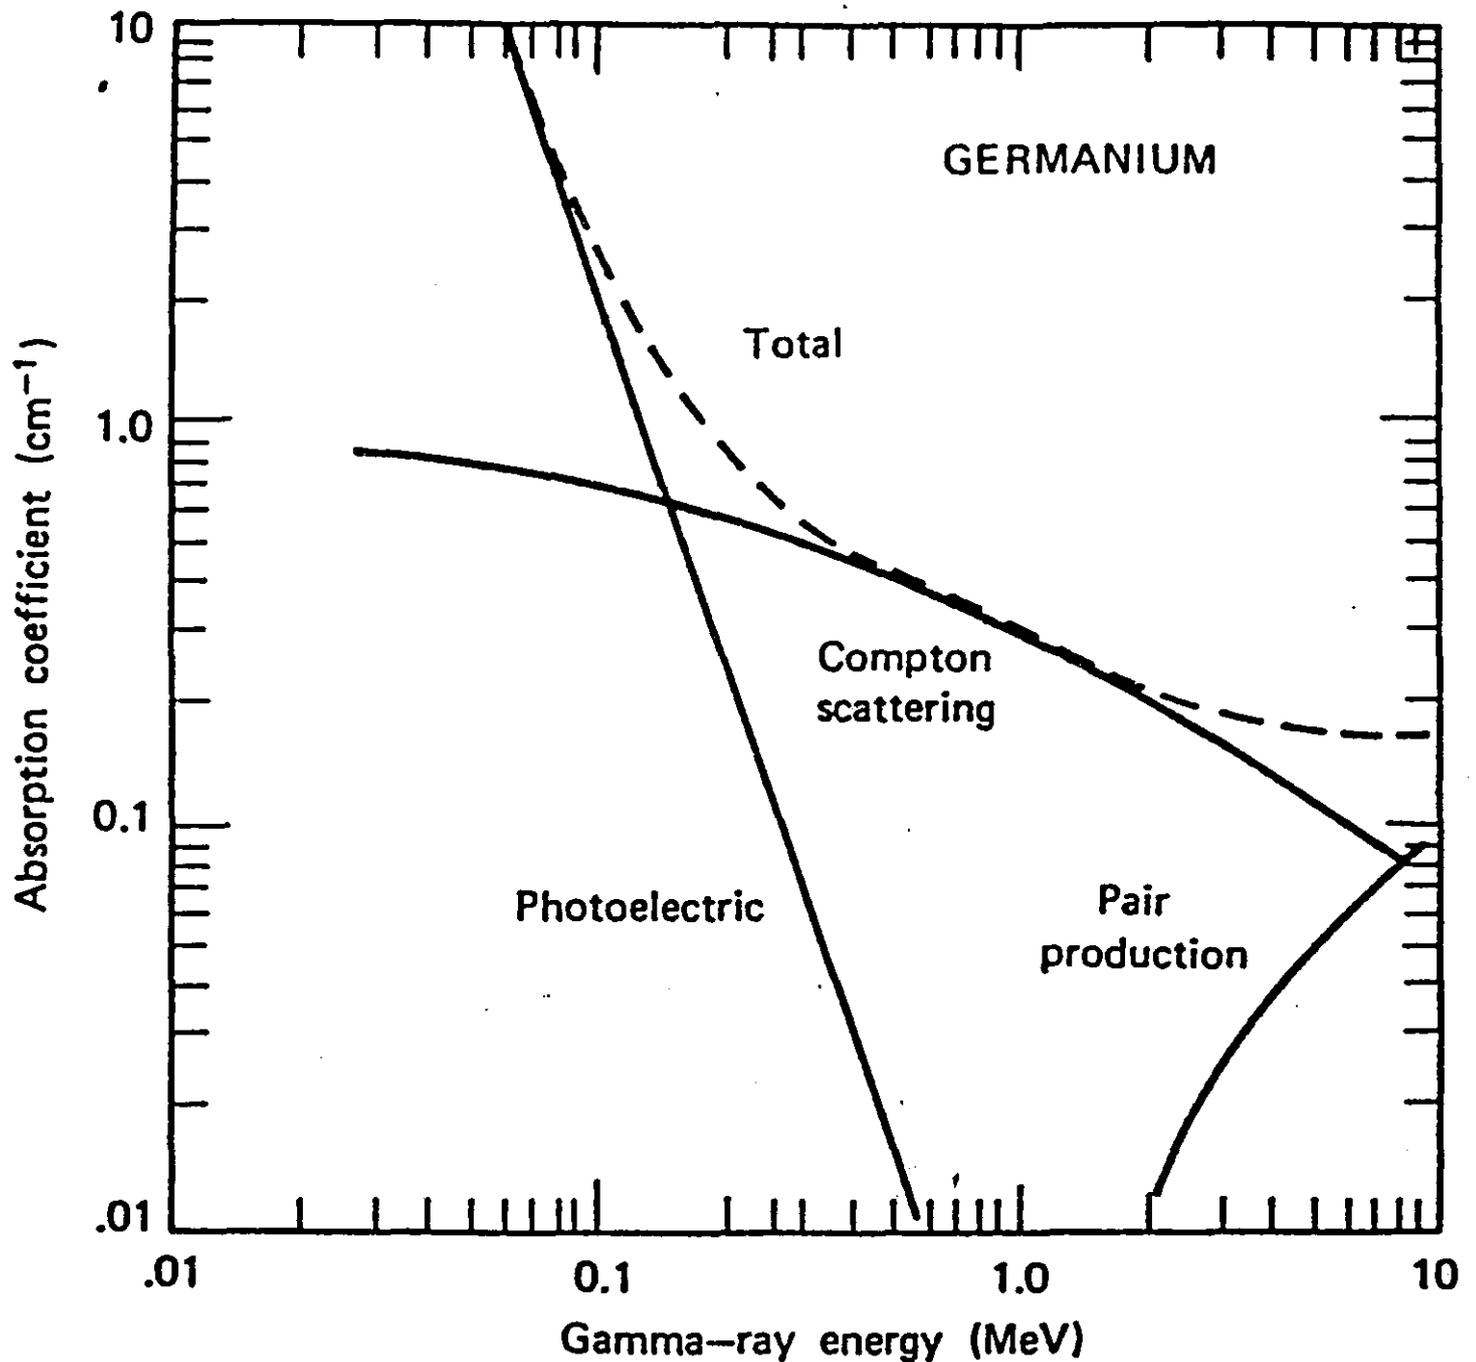


Figure 6.20 Partial and total absorption coefficients for gamma rays in germanium. [From G. Dearnaley and D. C. Northrop, *Semiconductor Counters for Nuclear Radiations* (Wiley, New York, 1966), p. 16.]

6.2c

6.5a

Fig. 2.10 Characteristics of an idealized counter as a function of voltage

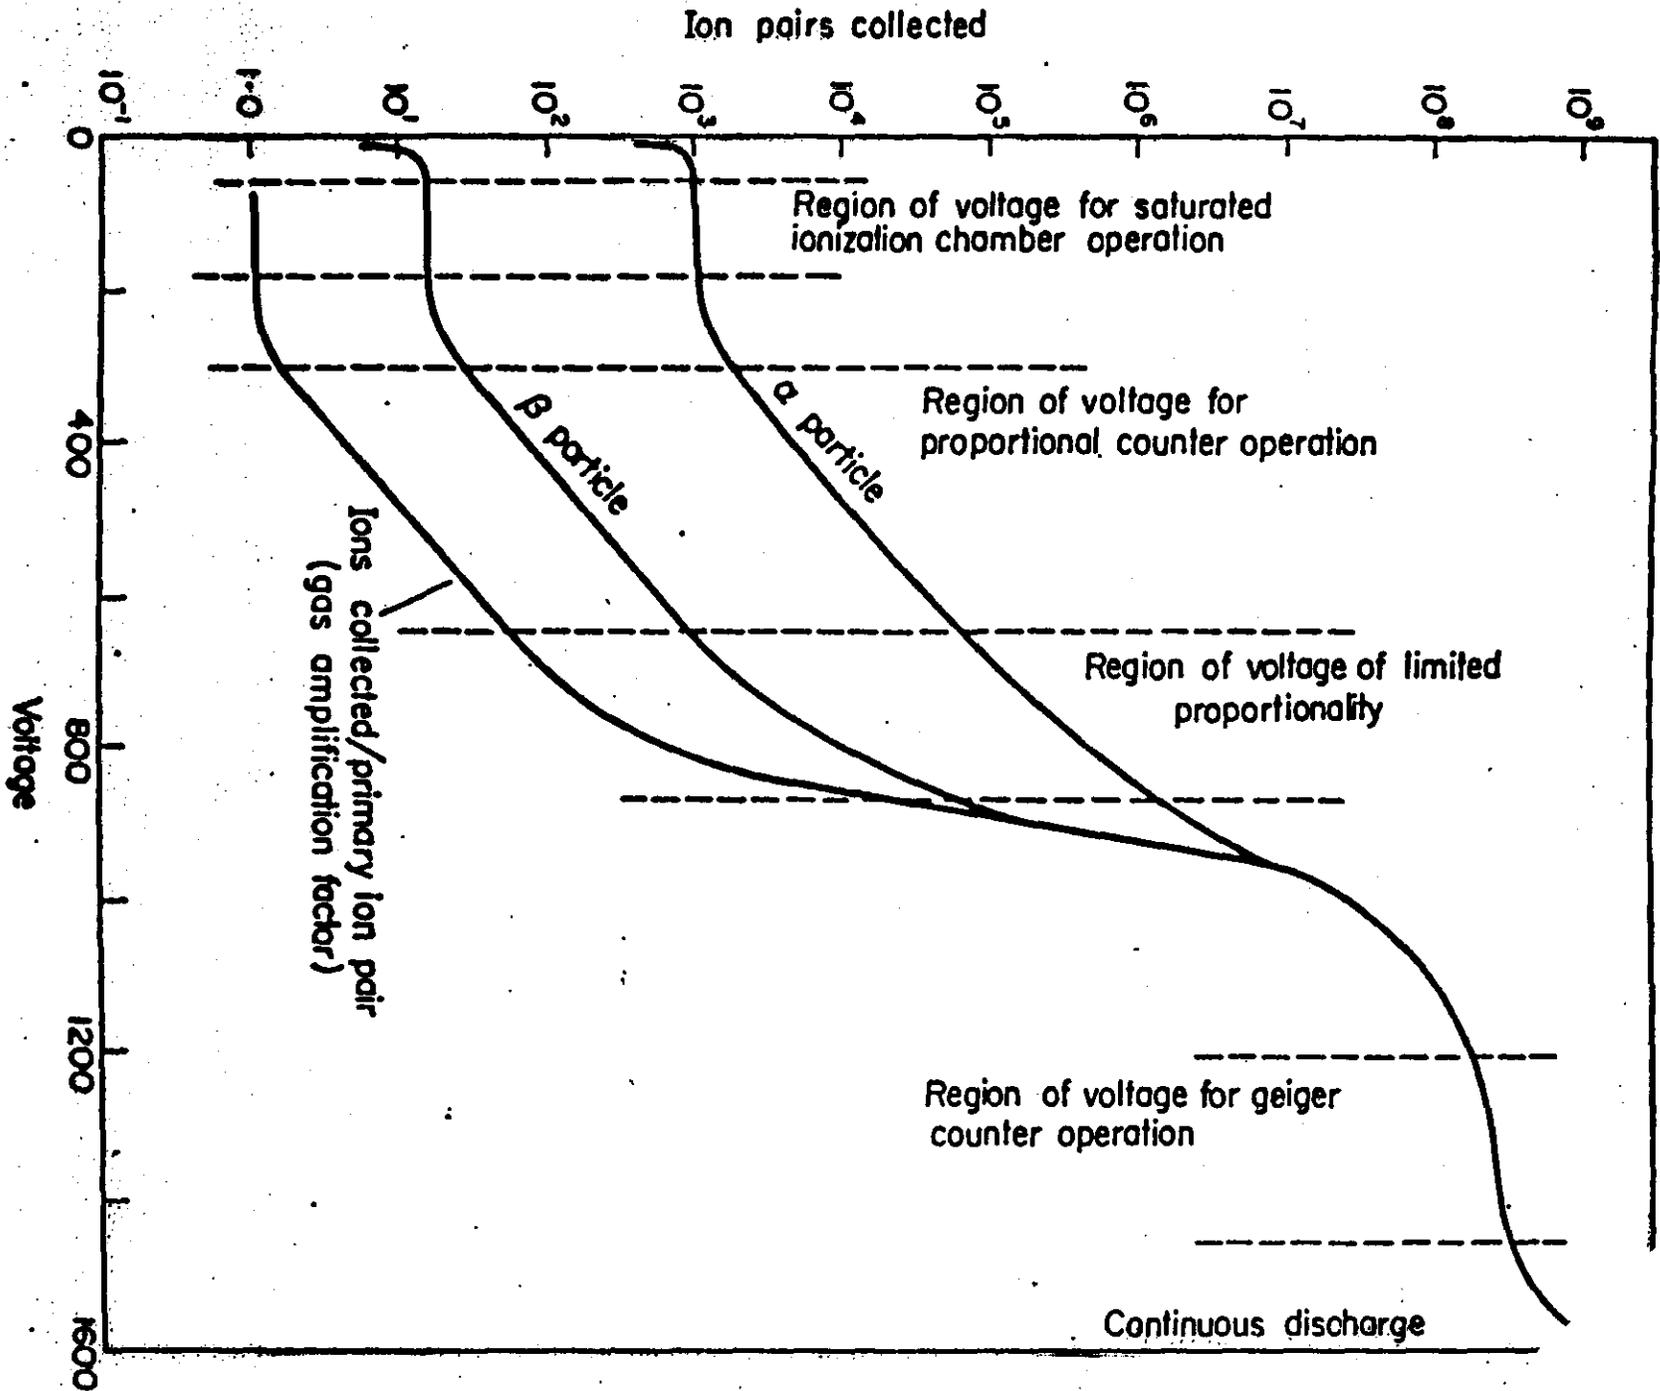

Activation Analysis: Practices

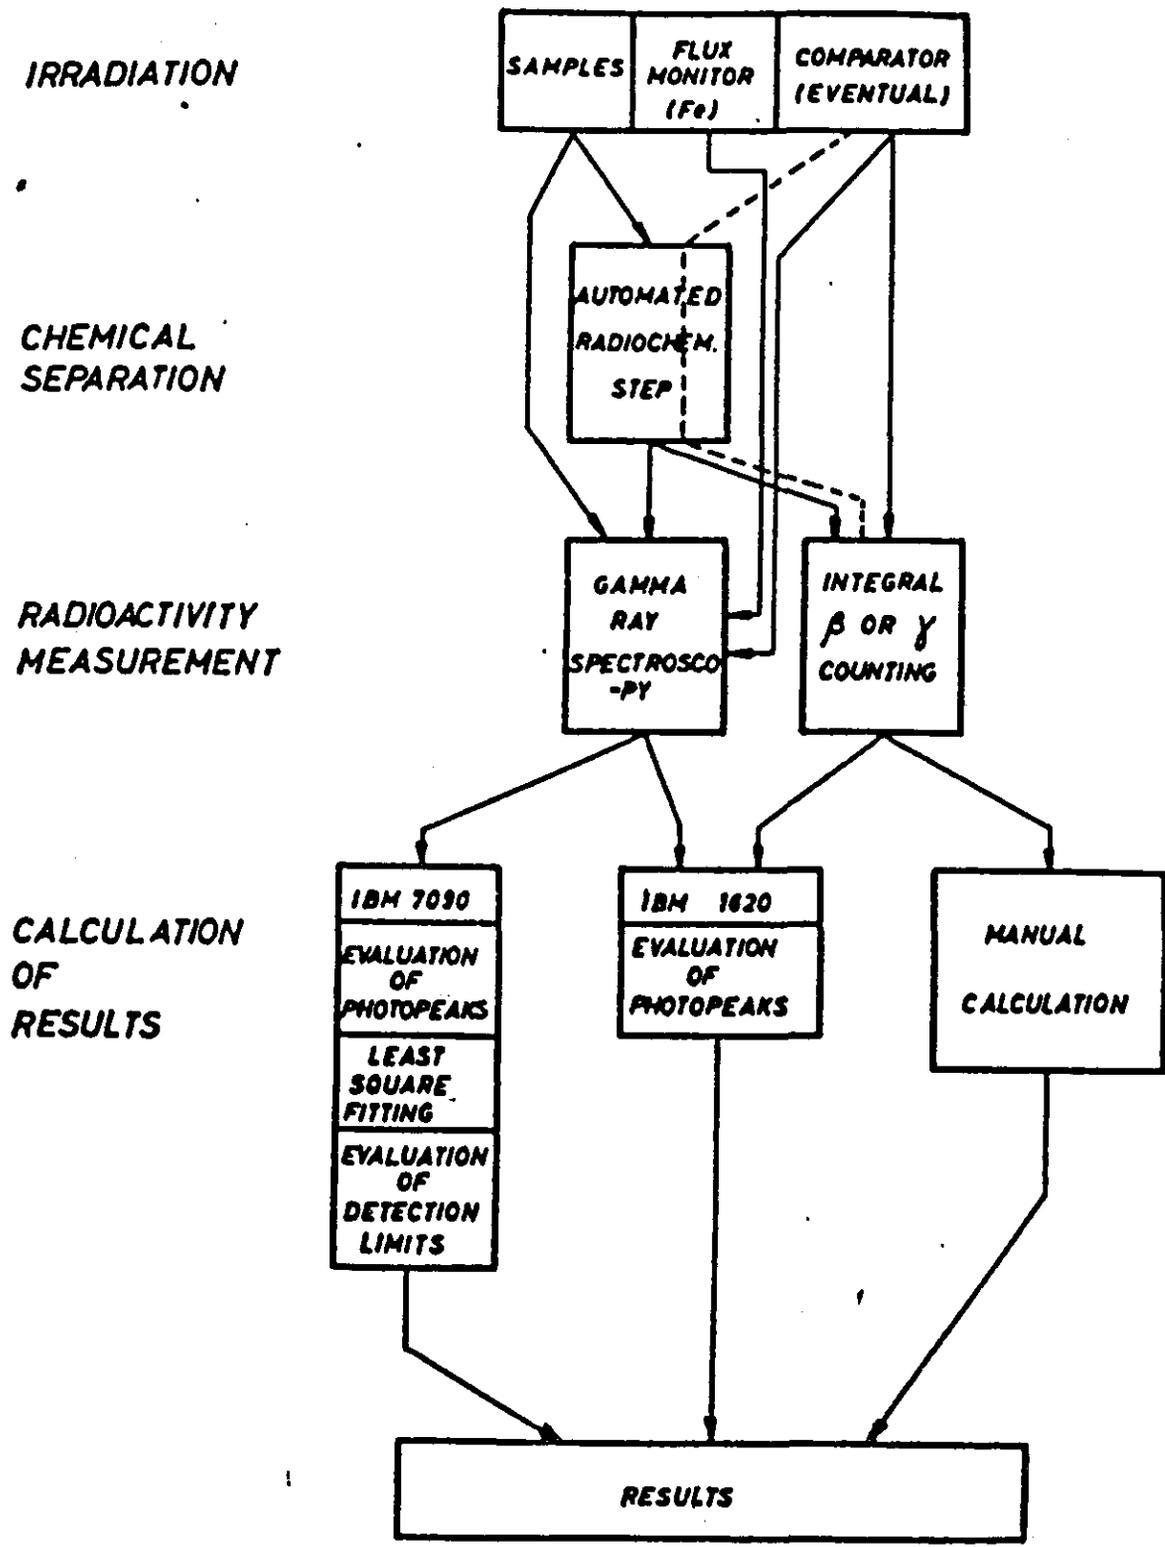


Figure 7.6 A flow sheet for an automated activation analysis system which includes radiochemical separations to concentrate the desired radionuclides or remove interfering radionuclides. [From F. Girardi, G. Guzzi, J. Pauly, and R. Pietra, The Use of an Automated System Including a Radiochemical Step in

6.302


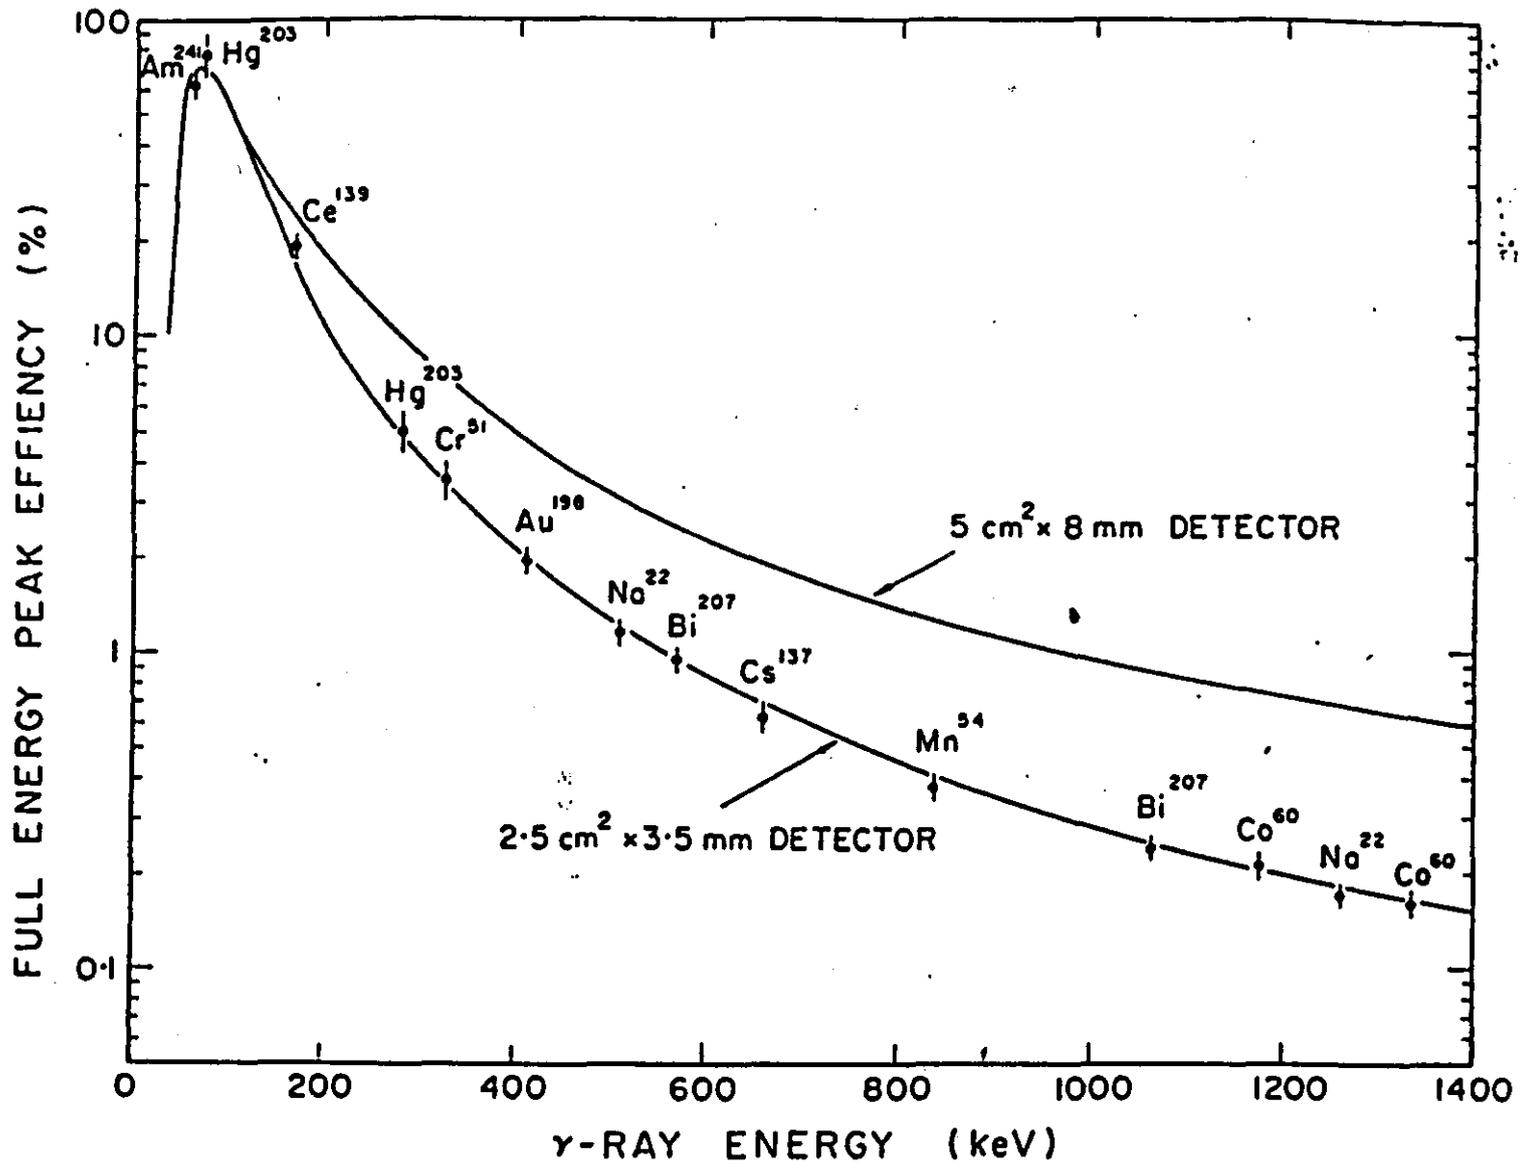


Figure 6.22 Full-energy peak efficiencies for two sizes of Ge(Li) detectors. At 1 MeV the efficiency of about 1% for the larger detector is almost four times that of the smaller detector. [From G. T. Ewan and A. J. Tavendale, High-resolution Studies of γ -Ray Spectra Using Li-Drift Germanium γ -Ray Spectrometers, *Can. J. Phys.* 42, 2286 (1964).]

6.3d

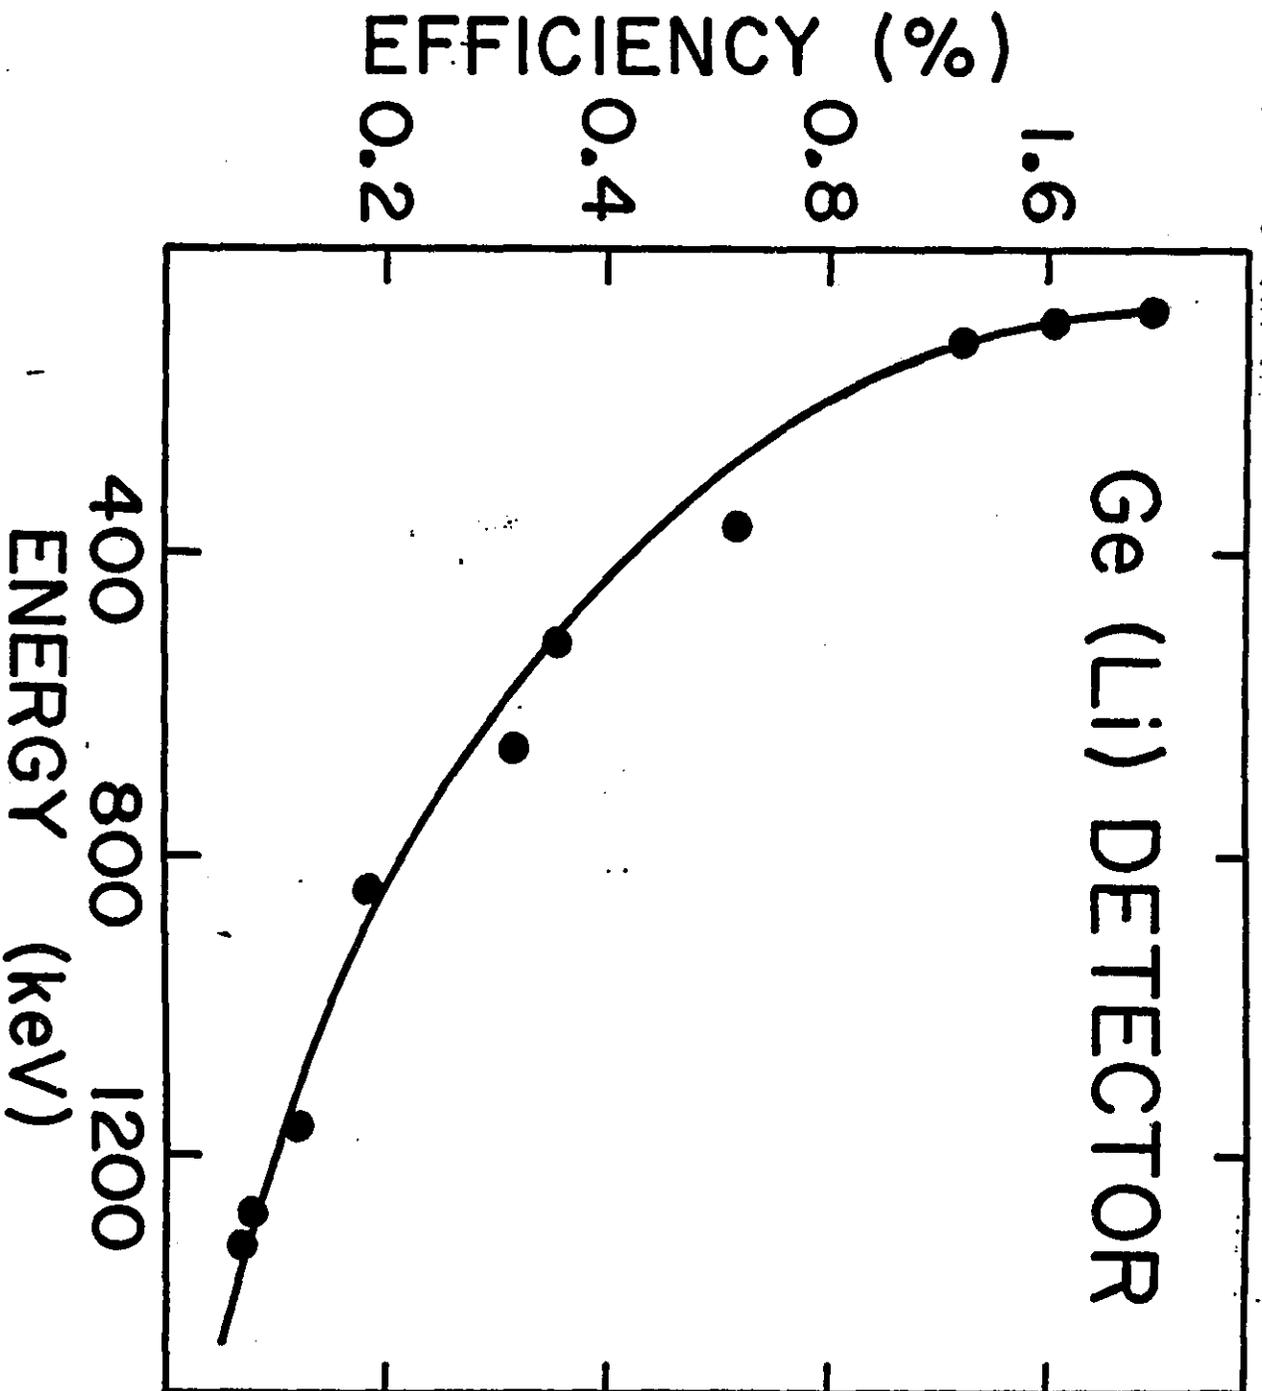

FULL-ENERGY PEAK EFFICIENCIES
OF A Ge(Li) DETECTOR

6.3d

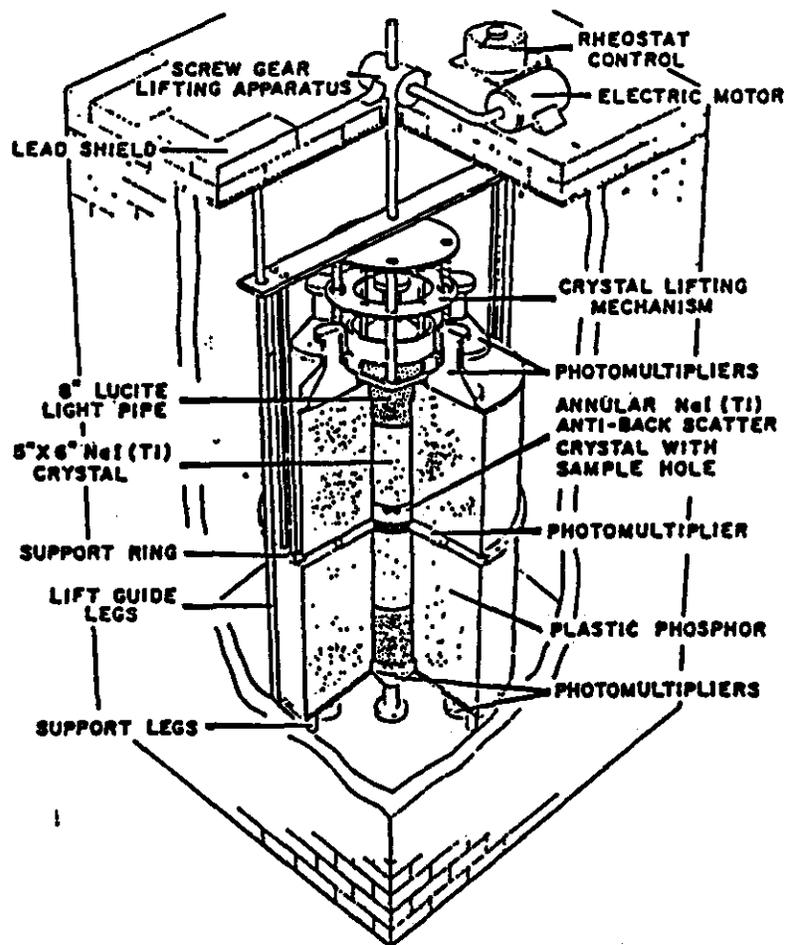
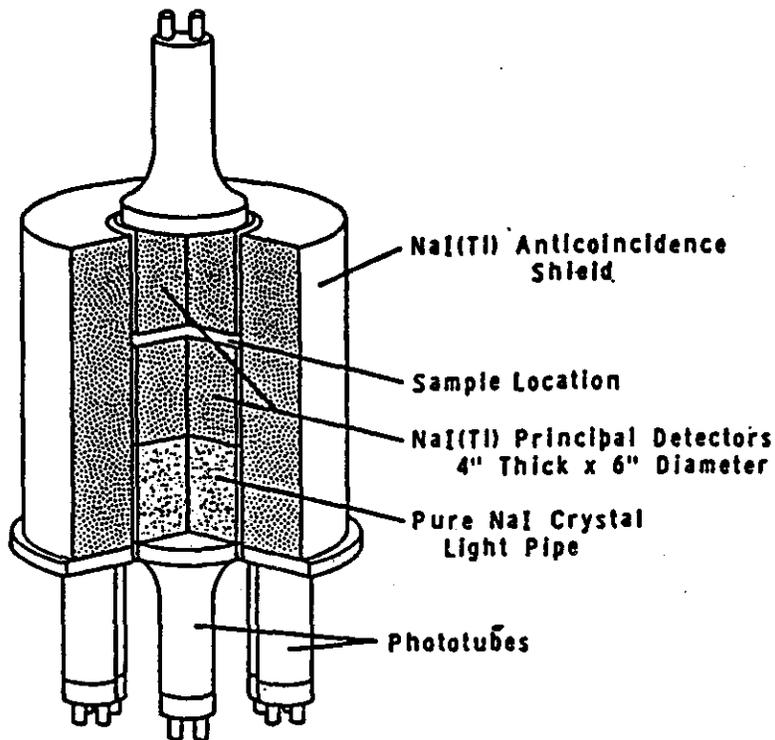


Figure 3.8 Cut-away views of a 2-NaI(Tl)-phosphor shield detector system for multidimensional gamma-ray spectrometry. [From R. W. Perkins and D. E. Robertson, in *Modern Trends in Activation Analysis* (Texas A&M University, College Station, 1965), pp. 48-57].

6.3e

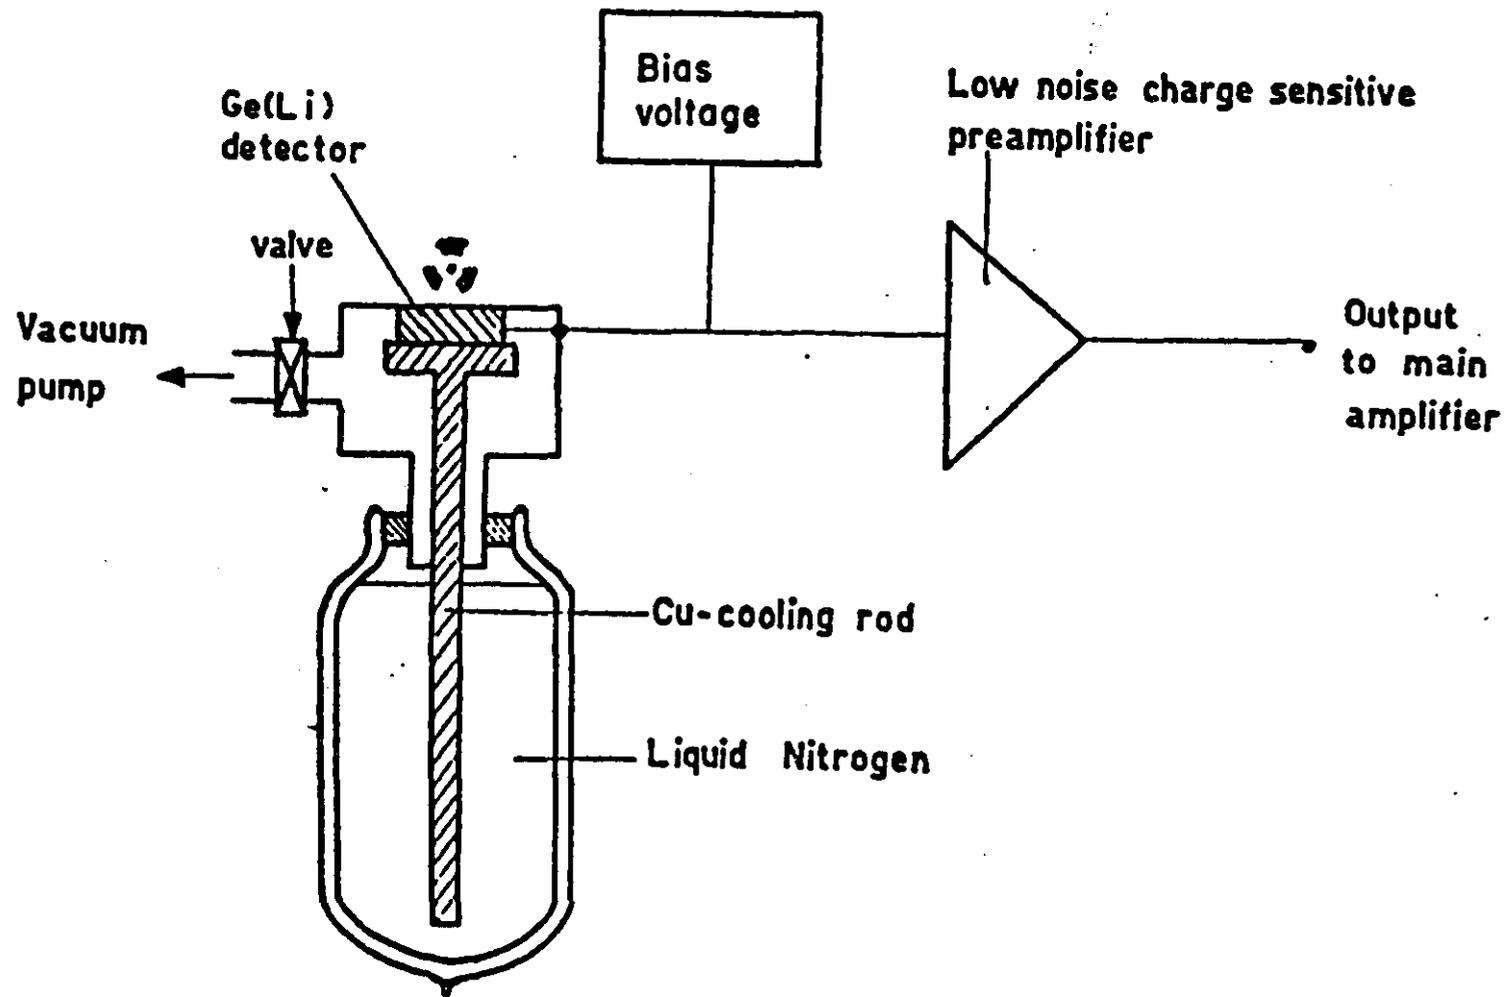


Fig. 6.23. Scheme of a typical Ge(Li) detector mounting.

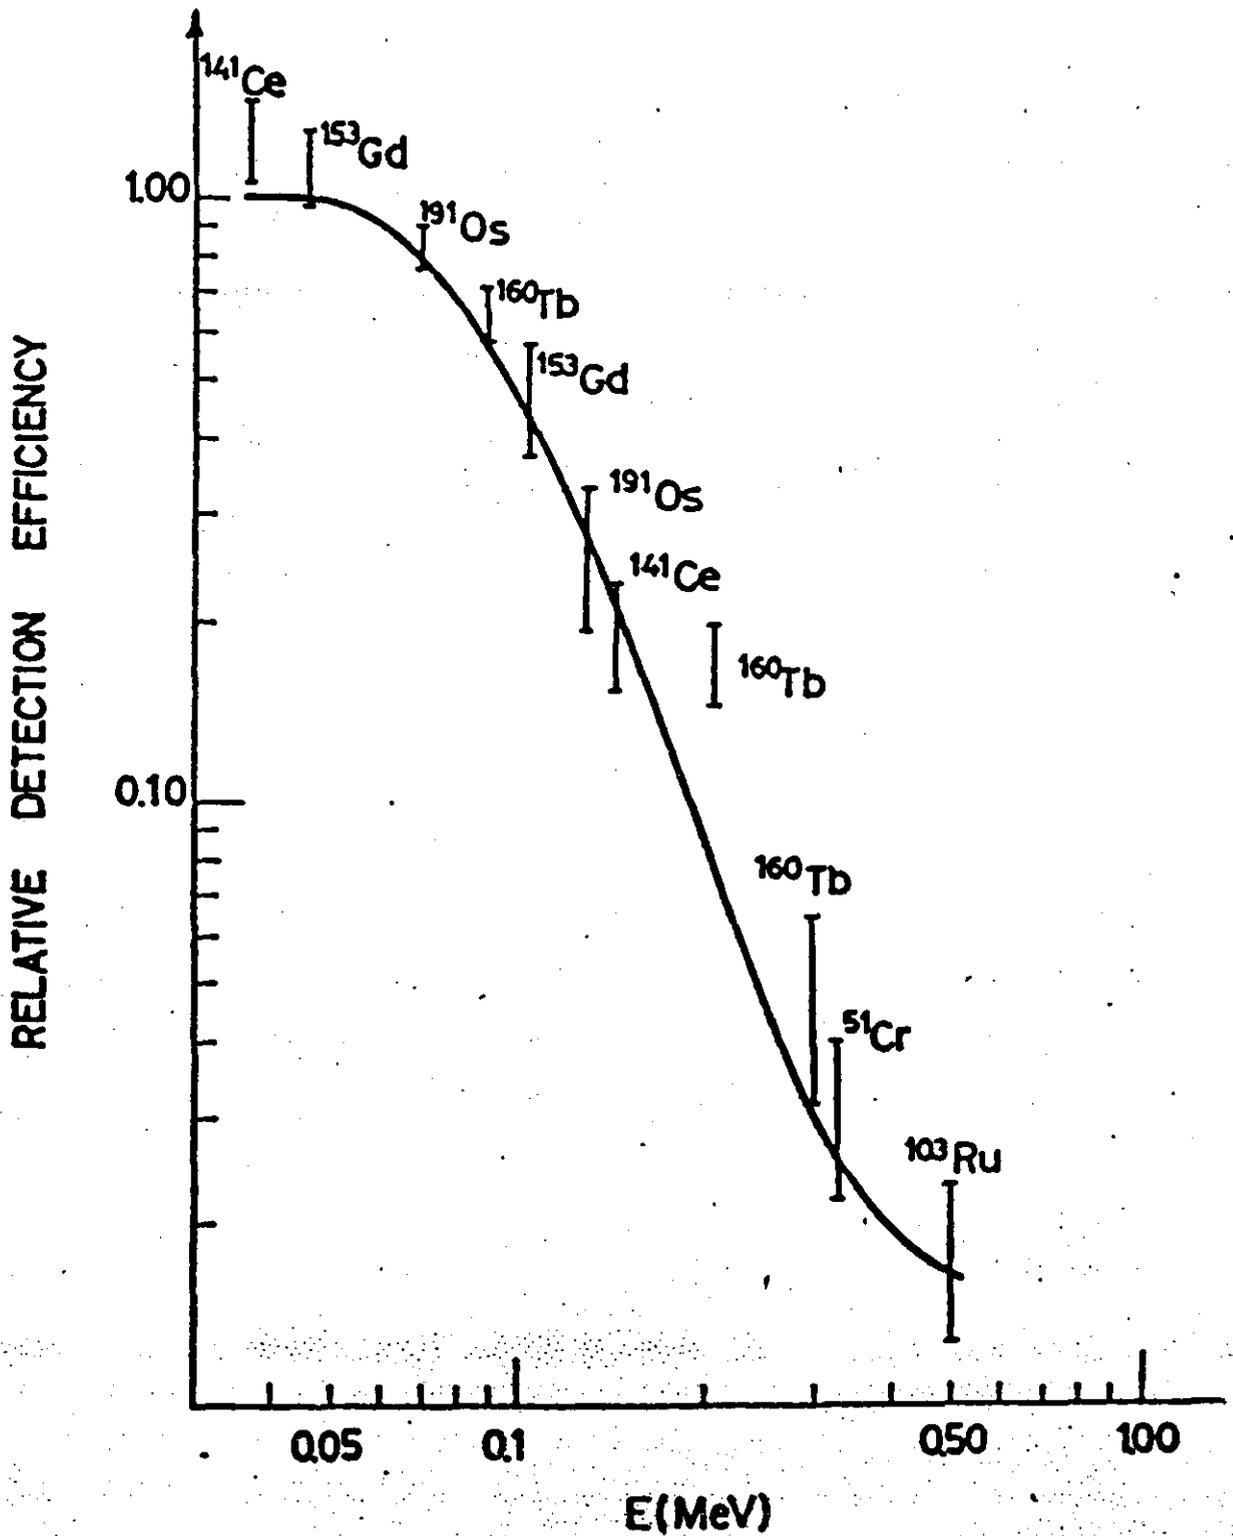


Fig. 6.25. Calculated photopeak detection efficiency ratio for a wafer of 7.5 cm diameter x 0.1 cm thickness, provided with a 37

6.3d

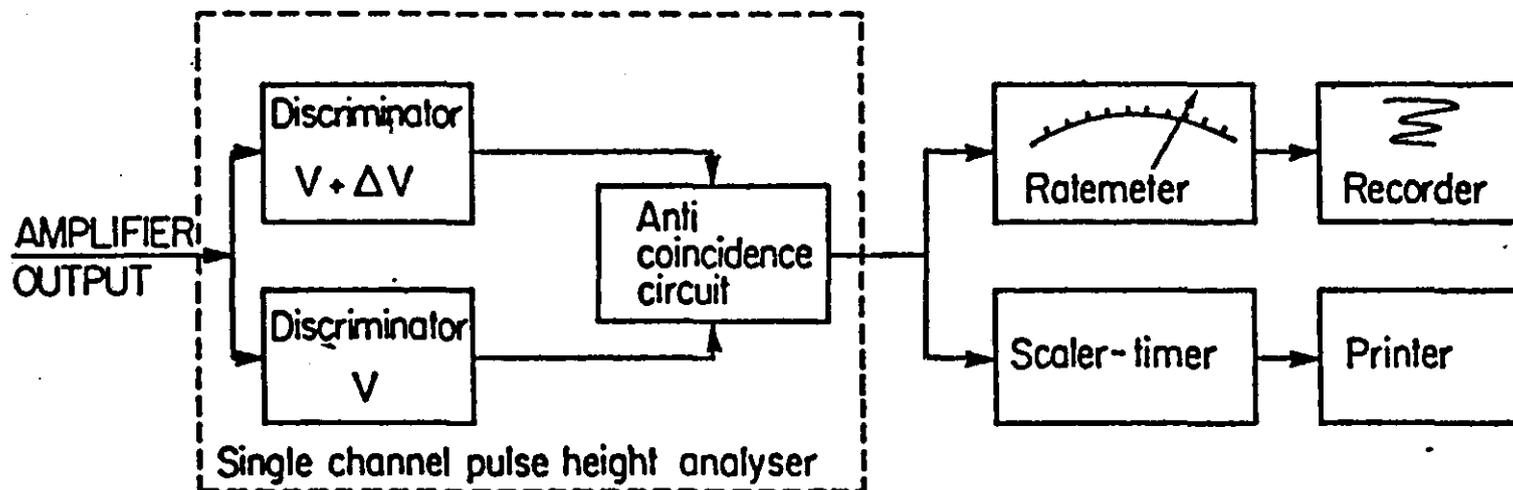


Fig. 6.26. Scheme of a single channel analyzer and related equipment.

C.B.d

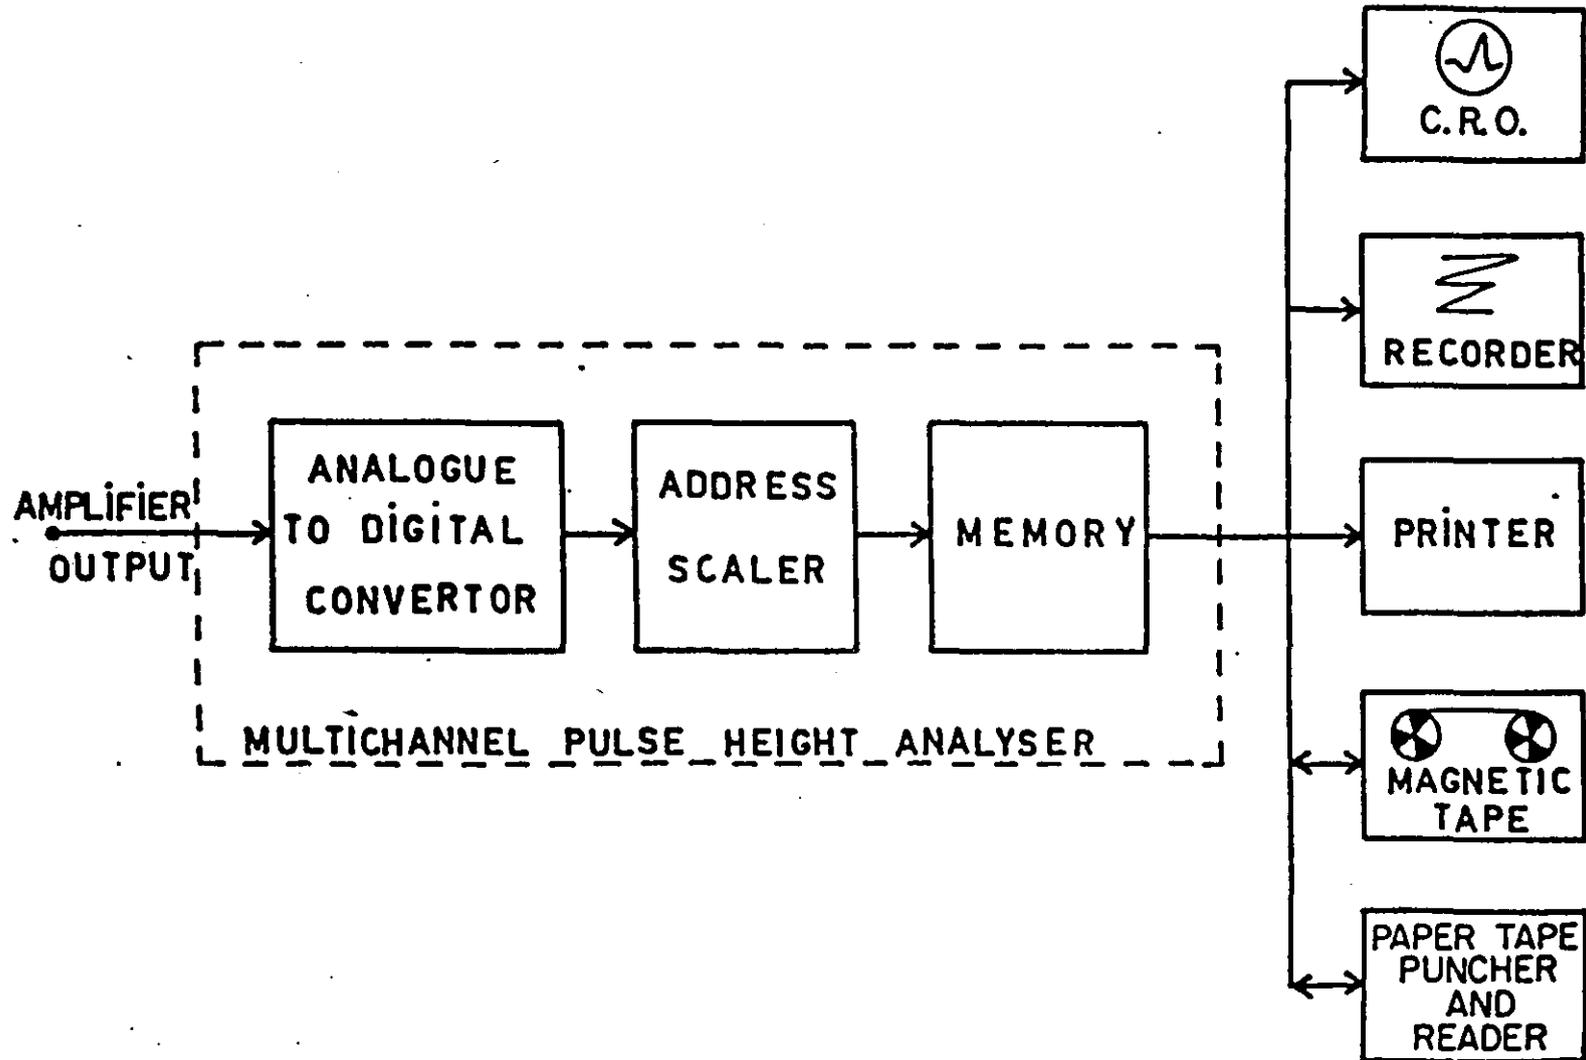


Fig. 6.27. Scheme of a multichannel analyzer and related equipment.

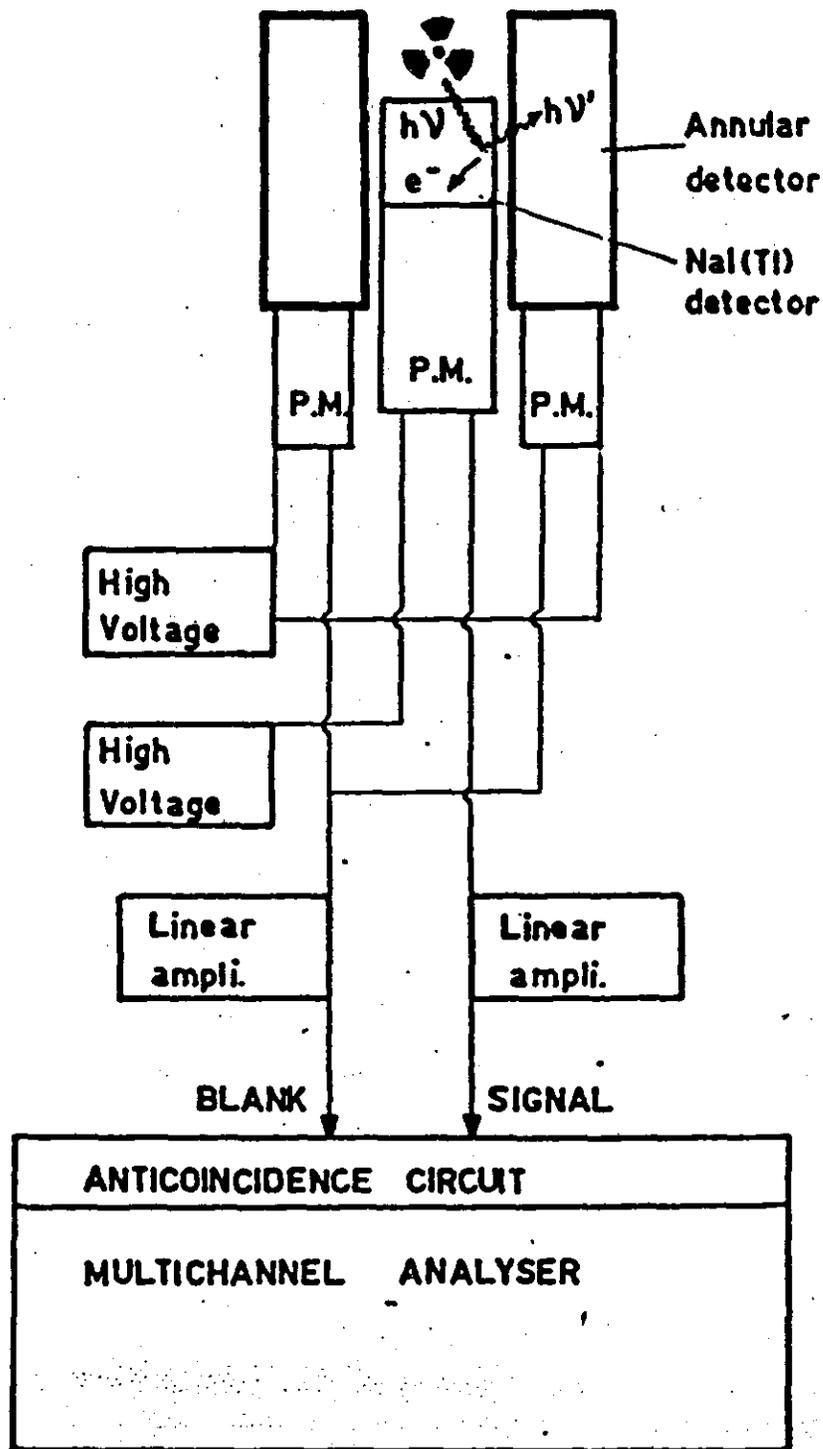


Fig. 6.36. Principle diagram of a Compton suppression spectrometer with an annular detector in anticoincidence.

6.3e

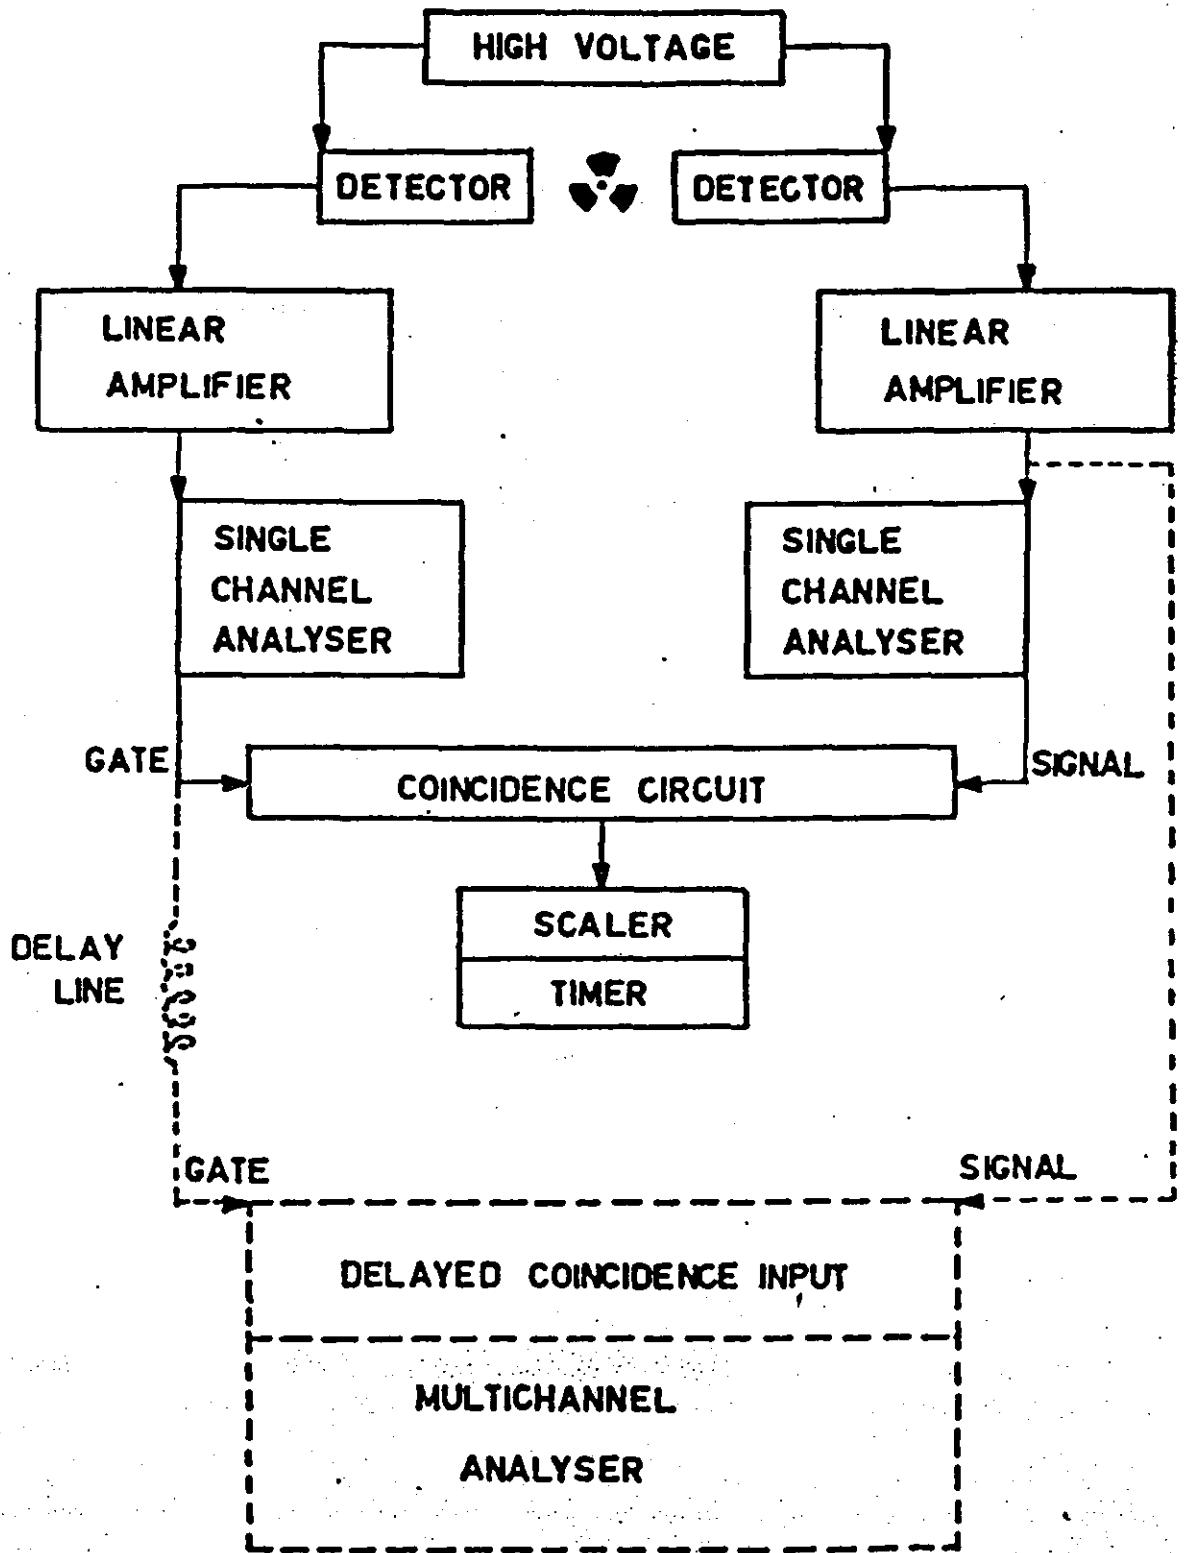


Fig. 6.32. Principle diagram of a "slow" coincidence spectrometer.

6.32

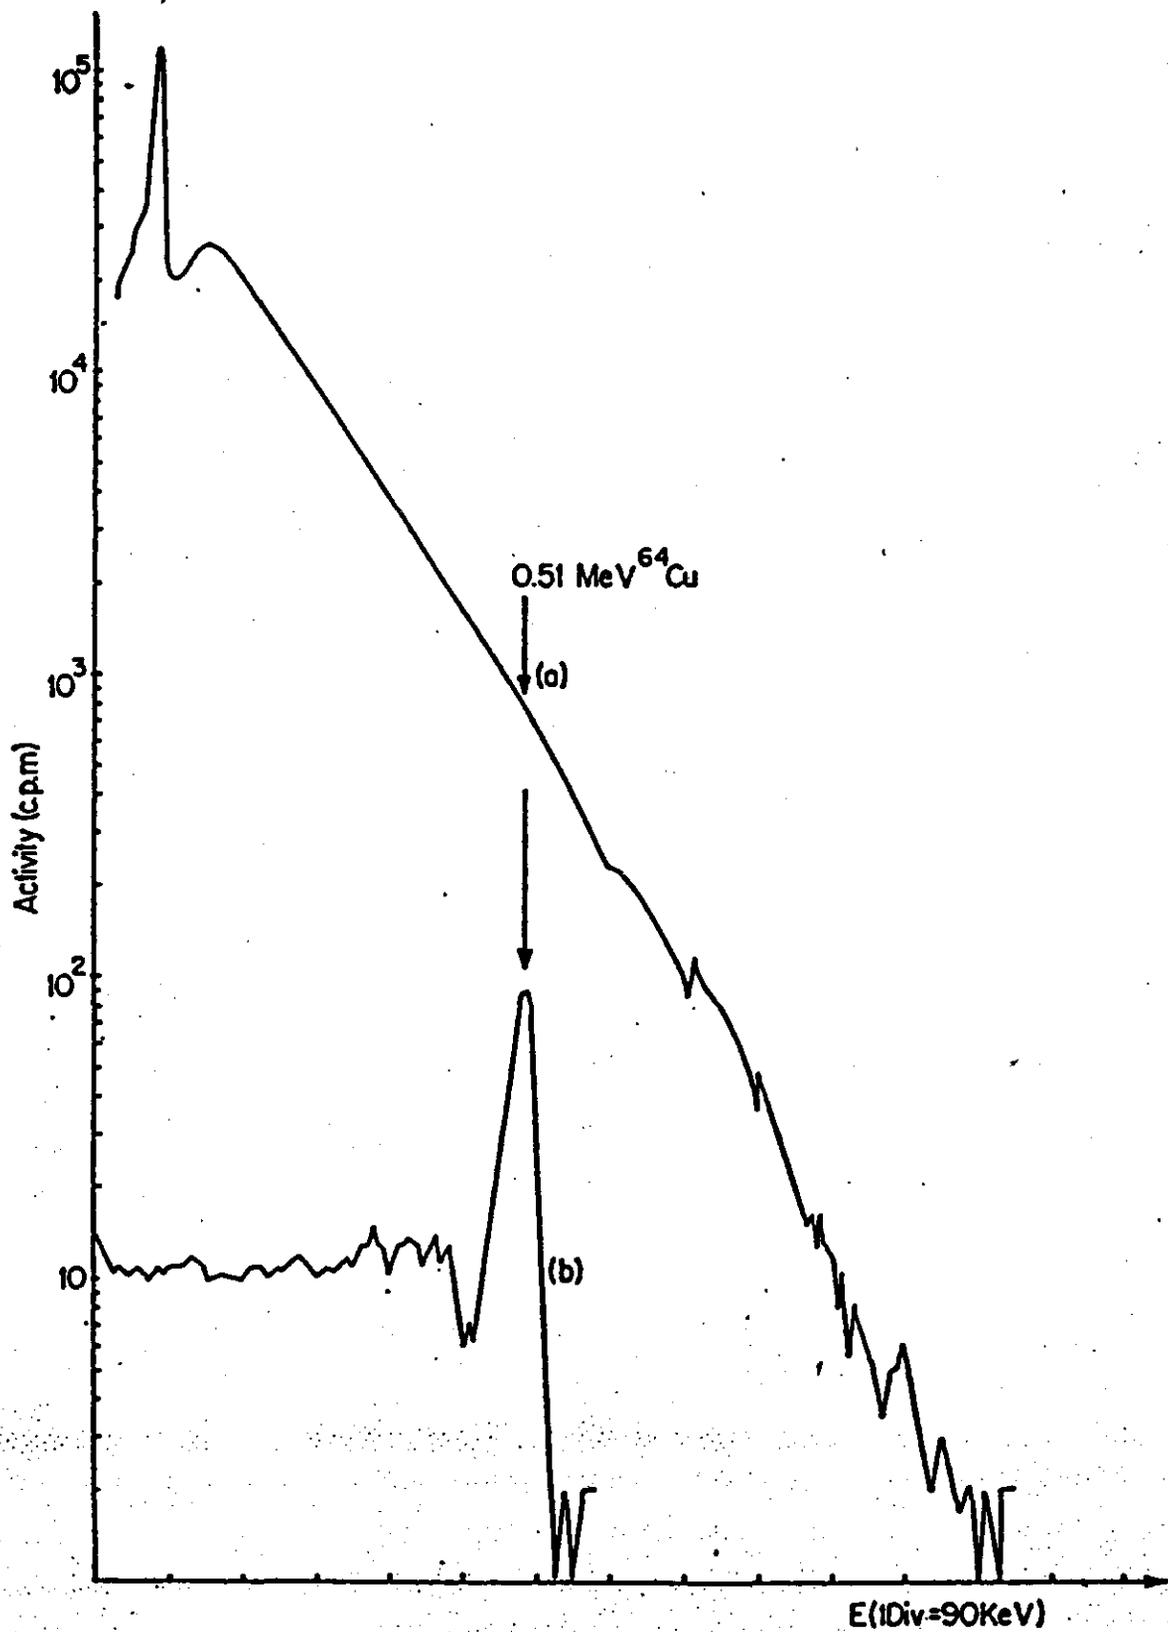


Fig. 6.34. Gamma spectrum of the ⁶⁴Cu annihilation radiation with the Bremsstrahlung spectrum of ²¹⁰Bi, measured without (a) and with (b) a coincidence technique in a neutron irradiated 1 g Bi sample, containing 0.226 ppm Cu (84).

h. Be